

A decorative wavy line in shades of gray and white, spanning the width of the page near the top.

Bante900P Portable Multiparameter Water Quality Meter

Instruction Manual

Introduction


Thank you for selecting the Bante900P portable multiparameter water quality meter. This manual provides a step-by-step guide to help you operate the meter, please carefully read the following instructions before use.

Unpacking


Before unpacking, ensure that the current work environment meets following conditions.

- Relative humidity is less than 80%.
- Ambient temperature is greater than 0°C and less than 60°C.
- No potential electromagnetic interference.


The following list describes the standard components of the meter. After the unpacking, please check all components are complete. If any are damaged or missing, please contact nearest distributor.

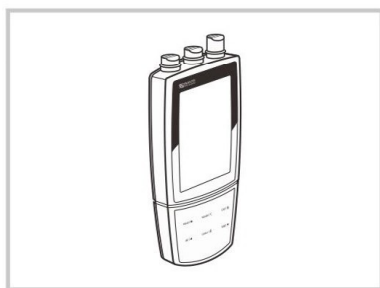

Bante900P Multiparameter Meter

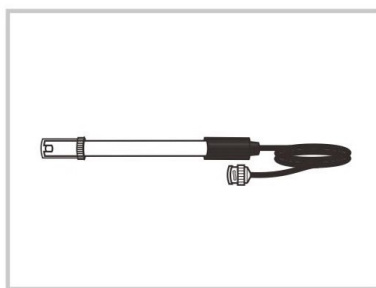


E201 pH Electrode

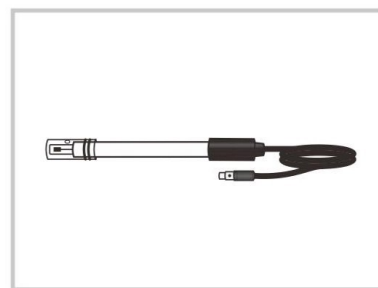


CON-1 Conductivity Electrode



DO100 Dissolved Oxygen Probe

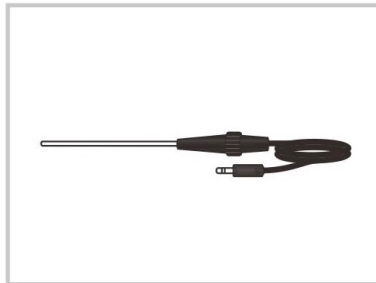

TP-10K Temperature Probe

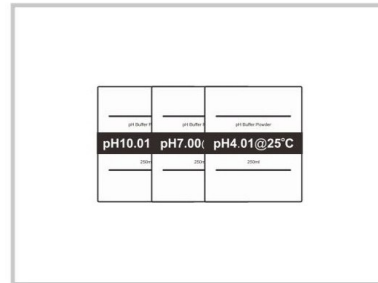

pH 10.01	pH 7.00	pH 4.01@25°C
10.01	7.00	4.01


pH Buffer Pouches



Conductivity Standard Solutions




DO Membrane Cap

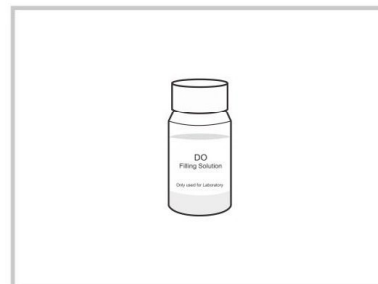







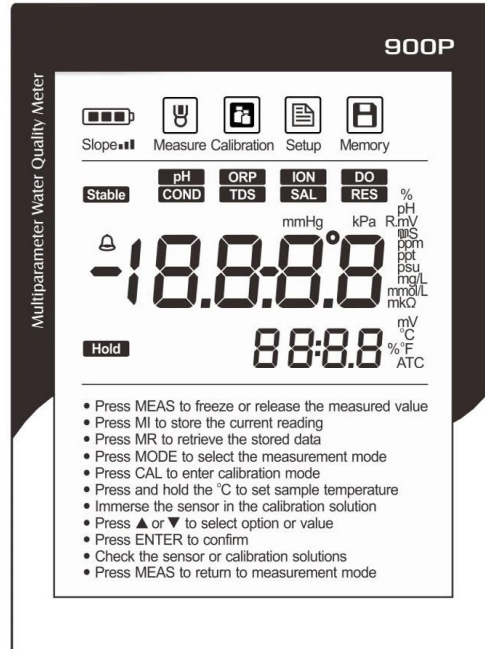

DO Electrolyte Solution

Display




The Bante900P multiparameter water quality meter is equipped with an easy-read LCD display that used to show the measured values and mode icons. The following table describes the function of each icon.




INDEX:

 Measure	Measurement mode icon: Indicates the meter is in the measurement mode.	 Low battery alarm: When the battery is depleted, the icon will disappear.
 Calibration	Calibration mode icon: Indicates the meter is in the calibration mode.	 Stable icon: Indicates the measuring value has stabilized.
 Setup	Setup mode icon: Indicates the meter is in the setting mode.	 Hold icon: Indicates the measuring value has been locked.
 Memory	Memory icon: Indicates the data is stored into memory.	 Calibration Due Alarm: Prompts the user to calibrate the meter.
Slope ■■■	Electrode slope icon: Indicates the average slope of the pH electrode.	ATC Automatic Temperature Compensation: Indicates the temperature compensation is enabled.

Keypad

KEY	FUNCTION
Meas 	<ul style="list-style-type: none"> • Switches the meter ON/OFF. • Locks the measured value, press the key again to resume measuring. • Exits the calibration or setting and returns to measurement.
Mode °C	<ul style="list-style-type: none"> • Toggles between available measurement modes. • Sets the temperature (Press and hold the key for 3 seconds).
Cal 	<ul style="list-style-type: none"> • Starts calibration. • Enters the setup menu (Press and hold the key for 3 seconds).
MI ▲	<ul style="list-style-type: none"> • Stores current reading to memory. • Increase value or scroll up through the menu item.
MR ▼	<ul style="list-style-type: none"> • Views the calibration report or data logs. • Decrease value or scroll down through the menu item.
Enter 	<ul style="list-style-type: none"> • Confirms the calibration, settings or displayed options. • Turn on/off the backlight (Press and hold the key for 3 seconds).

Connectors

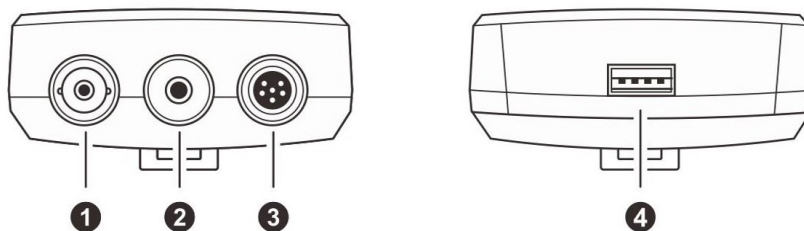


INDEX:

NO.	CONNECTOR	DESCRIPTION
1	BNC Connector	Used for connecting the pH, ORP or ion selective electrode
2	Phone Jack	Used for connecting the temperature probe
3	6-pin Connector	Used for connecting the conductivity electrode or dissolved oxygen probe
4	USB	Used for connecting the USB cable

Installing the Batteries

- Remove the battery cover from backside of the meter.
- Insert three AA batteries into the battery compartment, note polarity.
- Replace the battery cover into its original position. Installation is completed.




① When the batteries are depleted, the meter allows using the DC5V power adapter with USB cable for power supply. NOTE, take out the batteries.

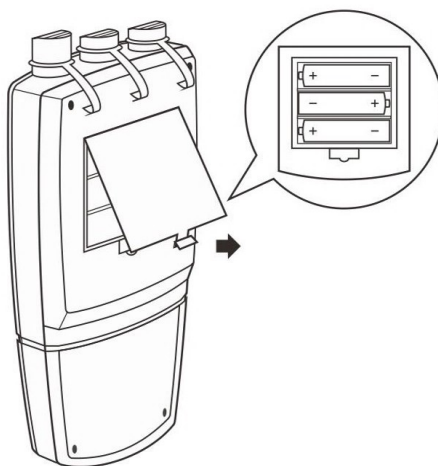

Connecting the Sensors

Take out the electrode from the carrying case.


- pH, ORP or Ion Selective Electrode: insert the connector into the BNC connector socket, rotate and push the connector clockwise until it locks.
- Conductivity Electrode or Dissolved Oxygen Probe: insert the connector into the 6-pin connector socket, ensure the connector is fully seated.
- Temperature Probe: insert the connector into to the corresponding connector socket.

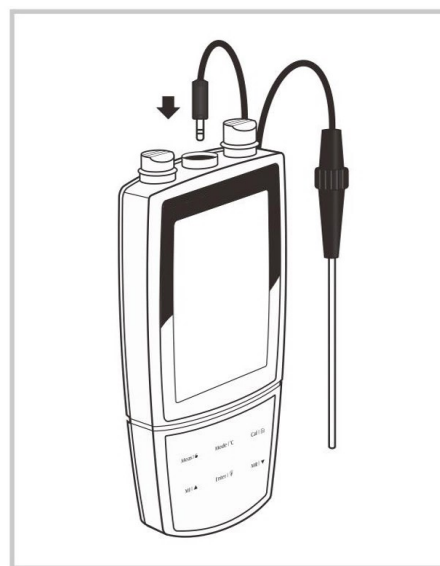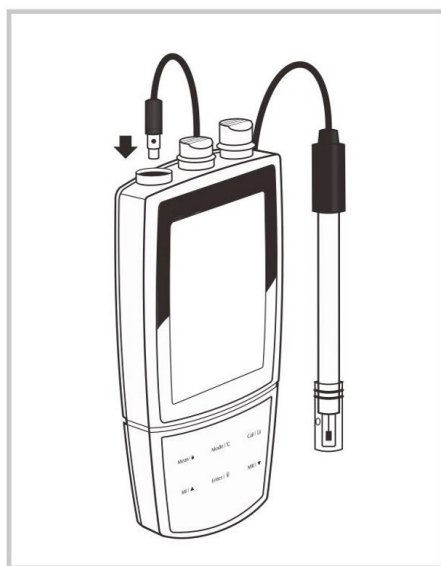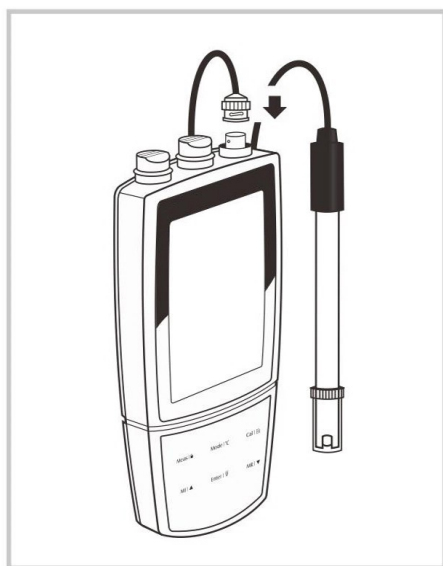

① After the connection is completed, DO NOT pull on the cable. Always make sure that connector is clean and dry.

Filling the Electrolyte Solution


1. Take out the electrolyte solution from the carrying case. Unscrew the membrane cap from the bottom of the dissolved oxygen probe.
2. Fill the membrane cap halfway with electrolyte solution.
3. Screw the membrane cap onto the probe, excess electrolyte solution will drain out.
4. Be sure the cathode of probe makes contact with membrane cap, the electrolyte solution in membrane cap should be without an air bubble.

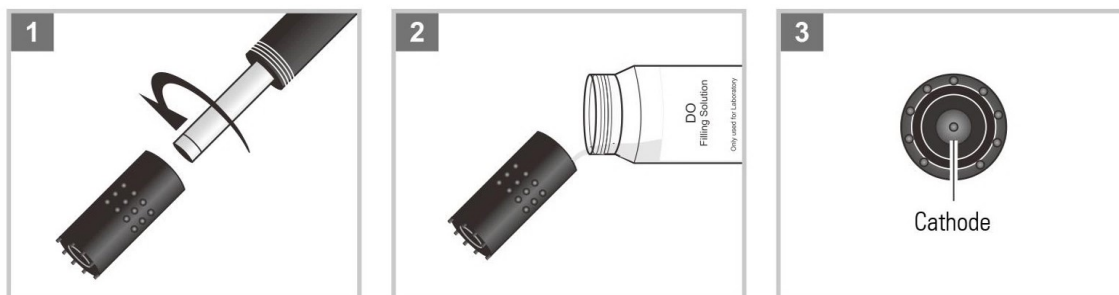


Prior to Use

Remove the protective cap from the bottom of the electrode.

- pH Electrode:
If the glass sensitive membrane has dried out, soak the electrode in 3M KCL solution (pH adjusted to 4.0) for at least 30 minutes.

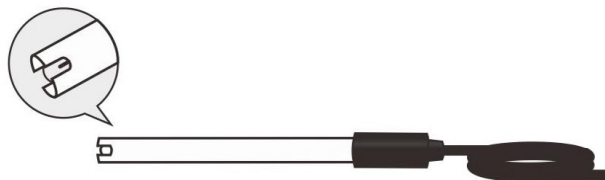

- ORP Electrode (purchase separately):
If the sensing element has dried out, soak the electrode in 4M KCL solution for at least 20 minutes.
- Ion Selective Electrode (purchase separately):
Soak the electrode in the 100ppm standard solution for at least 20 minutes.
- Conductivity Electrode:
Soak the electrode for a few minutes in tap water to remove dirt and oil stains on the electrode.

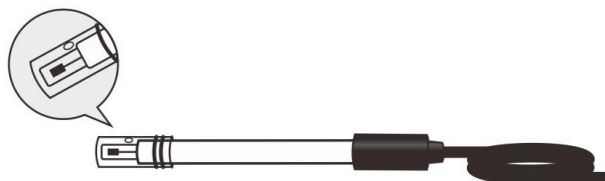

- Dissolved Oxygen Probe:
Connect the probe to meter, turn on the meter 10 to 15 minutes and wait for the probe to polarize.

Switching the Meter On and Off

- Press the **Meas** key to switch on the meter, the display shows the measured value.
- Press and hold the **Meas** key for 5 seconds, the meter will switch off.

Setup Menu

The Bante900P multiparameter water quality meter contains an integrated setup menu that is used to customize the displayed option to meet measurement requirements. In the different modes, the meter will show the corresponding options. The following table describes the functions of the menu items.

pH MODE:

MENU	DESCRIPTION	OPTIONS	DESCRIPTION	DEFAULT
bUF	pH Buffer: Set the pH buffer group for calibration and auto-recognition.	USA	USA (pH1.68/4.01/7.00/10.01/12.45)	USA
		NIST	NIST (pH1.68/4.01/6.96/9.18/12.45)	
		DIN	DIN (pH1.09/4.65/6.79/9.23/12.75)	
		USER	User-Defined	
CAL	Calibration Points: Set the number of calibration points.	1	1 point	3 points
		2	2 points	
		3	3 points	
		4	4 points	
		5	5 points	
RESO	Resolution: Set the resolution of the pH measurement.	0.001	0.001pH	0.001pH
		0.01	0.01pH	
		0.1	0.1pH	
UNIT	Measurement Unit: Set the default temperature unit.	°C	Degrees Celsius	°C
		°F	Degrees Fahrenheit	

ORP MODE:

MENU	DESCRIPTION	OPTIONS	DESCRIPTION	DEFAULT
RESO	Resolution: Set the resolution of the ORP measurement.	0.1	0.1mV	0.1mV
		1	1mV	

ION MODE:

MENU	DESCRIPTION	OPTIONS	DESCRIPTION	DEFAULT
UNIT	Measurement Unit: Set the ion concentration and temperature units.	ppm	Parts per million	ppm, °C
		mg/L	Milligrams per liter	
		mol/L	Moles per liter	
		°C	Degrees Celsius	
		°F	Degrees Fahrenheit	

CAL	Calibration Points: Set the number of calibration points.	2	2 points	2 points
		3	3 points	
		4	4 points	
		5	5 points	
ION	Ionic Valency: Set the ion valence of sample.	1	Monovalent	Monovalent
		2	Divalent	

CONDUCTIVITY/TDS/SALINITY/RESISTIVITY MODE:


MENU	DESCRIPTION	OPTIONS	DESCRIPTION	DEFAULT
CELL	Cell Constant: Set the cell constant to match connected electrode.	0.1	K=0.1	K=1
		1	K=1	
		10	K=10	
		USER	User-Defined	
COE	Temperature Coefficient: Set the linear temperature compensation coefficient.	2.10	Range: 0.0~10.0%/°C	2.10
CAL	Calibration Points: Set the number of calibration points.	1	1 point	1 point
		2	2 points	
		3	3 points	
		4	4 points	
		5	5 points	
PURE	Pure Water Coefficient: When the option is enabled, pure water coefficient will be applied automatically for ultra-pure water measurements.	YES	Enable	Disable
		NO	Disable	
Std	Reference Temperature: Set the normalization temperature for conductivity measurement and calibration.	25°C	25°C	25°C
		20°C	20°C	
TDS	TDS Factor: Set the default TDS conversion factor.	0.5	Range: 0.40~1.00	0.5
UNIT	Measurement Unit: Set the default temperature unit.	°C	Degrees Celsius	°C
		°F	Degrees Fahrenheit	

DISSOLVED OXYGEN MODE:


MENU	DESCRIPTION	OPTIONS	DESCRIPTION	DEFAULT
CAL	Calibration Points: Set the number of calibration points.	1	1 point	1 point
		2	2 points	
PRES	Pressure Coefficient: Set the barometric pressure coefficient.	760	Range: 450~850mmHg or 60.0~113.3kPa	760mmHg
SAL	Salinity Coefficient: Set the salinity coefficient.	0.0	Range: 0.0~50.0ppt	0.0ppt
RESO	Resolution: Set the resolution of the DO measurement.	0.01	0.01mg/L (0.1%)	0.01mg/L
		0.1	0.1mg/L (1%)	
UNIT	Measurement Unit: Set the default measurement units.	°C	Degrees Celsius	°C mg/L mmHg
		°F	Degrees Fahrenheit	
		mg/L	Milligrams per liter	
		ppm	Parts per million	
		mmHg	Pressure unit	
		kPa	Pressure unit	


GENERAL OPTIONS:


MENU	DESCRIPTION	OPTIONS	DESCRIPTION	DEFAULT
STAB	Stability Criteria: When the LO option is enabled, the Stable icon will quickly appear on the display. When the HI option is enabled, the icon will take longer to appear, but guarantees high accuracy of the measurement.	LO	Low	Low
		HI	High	
HOLD	Auto-Hold: When the option is enabled, the meter will automatically sense a stable reading and lock the measurements.	YES	Enable	Disable
		NO	Disable	
OFF	Auto-Power Off: When the option is enabled, the meter will automatically turn off if no key is pressed within a specified time period.	10	10 minutes	Disable
		20	20 minutes	
		30	30 minutes	
		NO	Disable	

CALL	Calibration Due: When the option is enabled, if the meter does not calibrated within a specified time period, the meter will automatically show the  icon.	1...31	1 to 31 days	Disable
		OFF	Disable	
DATE	Date and Time: Set the current date and time.	---	Year-month-day, hour-minutes	
CLR	Clear Stored Data: Delete all stored readings in the memory.	YES	Enable	Disable
		NO	Disable	
rSt	Factory Reset: If enabled, all of the calibration data and selected parameters will back to factory default settings, the meter must be recalibrated.	YES	Enable	Disable
		NO	Disable	


Setting the default option


- 1.1 If necessary, press the **Mode** key until the display shows desired measurement mode (e.g., pH).
- 1.2 Press and hold the  key for 3 seconds to enter the setup menu and the **▲** or **▼** key to select the menu item (e.g., BUF/P-01).
- 1.3 Press the **Enter** key, the display shows an option.
- 1.4 Press the **▲** or **▼** key to select the desired option.
- 1.5 Press the **Enter** key to confirm, the meter returns to the measurement mode. Setting is completed.

 If you want to exit the setting, press the **Meas** key.

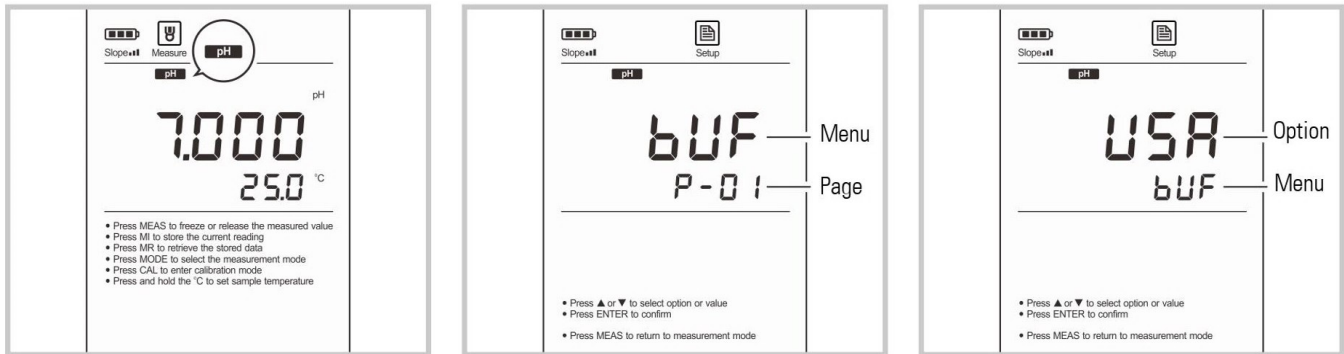

Setting the date and time

- 2.1 Press and hold the  key for 3 seconds to enter the setup menu and the **▲** or **▼** key until the display shows "DATE".
- 2.2 Press the **Enter** key, the meter shows current year (e.g., 2018).
- 2.3 Press the **▲** or **▼** key to set year and the **Enter** key to confirm, the display shows current date and time (Format: month-day, hour-minutes).
- 2.4 Press the **▲** or **▼** key to set the date and time, press the **Enter** key to confirm until the meter returns to the measurement mode. Setting is completed.

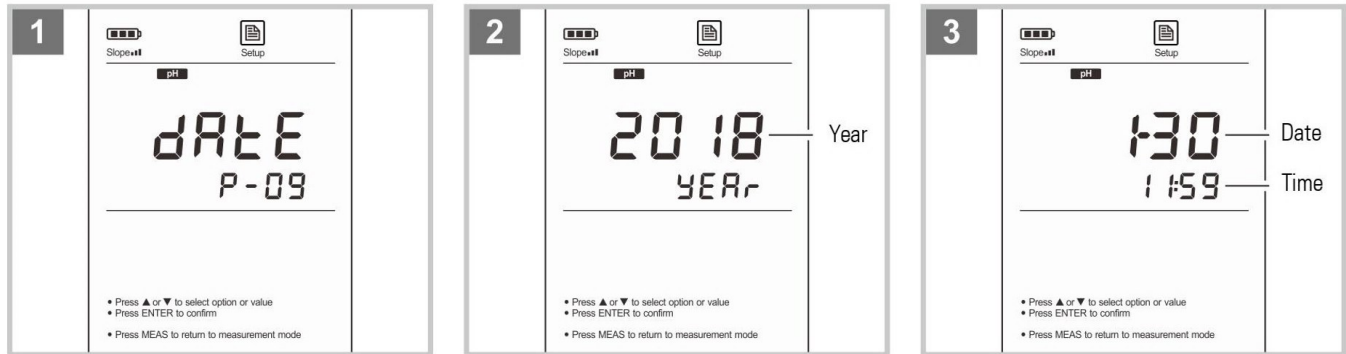


Temperature Compensation

In order to get accurate measuring results, we recommend that using a temperature probe for the calibration and measurements. Note, the dissolved oxygen probe has a built-in temperature sensor. You do not need to use the supplied temperature probe.

Automatic Temperature Compensation

Connect the temperature probe to the meter (Refer to page 4 "Connecting the Sensors"). The ATC icon immediately appears on the display, the meter is now switched to the automatic temperature compensation mode.

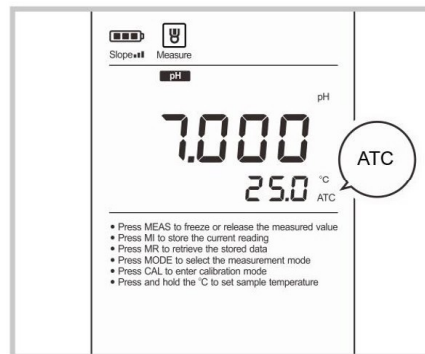

Manual Temperature Compensation

If the meter does not detect a temperature probe, the °C icon will show on the display indicating that the meter is switched to the manual temperature compensation mode. To set the temperature value of sample, follow the steps below.

1. Press and hold the °C key for 3 seconds to enter the temperature setting mode.
2. Press the ▲ or ▼ key to modify the temperature value.
3. Press the **Enter** key to confirm.

- i** Press the ▲ or ▼ key once, the setting value will increase or decrease by 0.1. Press and hold the ▲ or ▼ key, the setting value will increase or decrease by 1.

pH Calibration


The Bante900P multiparameter water quality meter allows 1 to 5 points calibration in the pH mode. We recommend that you perform at least 2 points calibration for high accuracy measurement. The meter will automatically recognize and calibrate to following standard buffer values.

USA Standard Buffers	pH1.68, 4.01, 7.00, 10.01, 12.45
NIST Standard Buffers	pH1.68, 4.01, 6.86, 9.18, 12.45
DIN Standard Buffers	pH1.09, 4.65, 6.79, 9.23, 12.75


If the USER option is selected, the meter will allow only 2 points calibration. Single point calibration should only be carried out with pH7.00, 6.86 or 6.79, otherwise calibration will not be accepted.

Make sure to calibrate the meter when attaching a new electrode or during first use. DO NOT reuse the calibration solution after calibration, contaminants in solution will affect the calibration and eventually the accuracy of the measurement.


Single point calibration

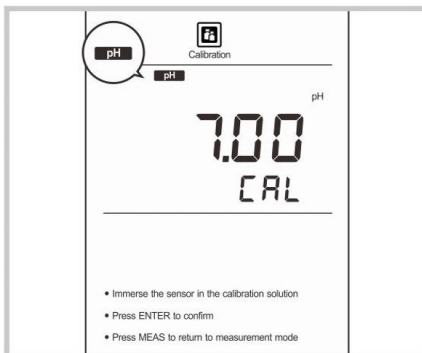

- 1.1 Press the **Mode** key until the meter shows **pH** icon and you have selected 1 point calibration in the setup menu.
- 1.2 Press the **Cal** key, the display shows pH7.00/CAL (or 6.86/CAL, or 6.79/CAL).

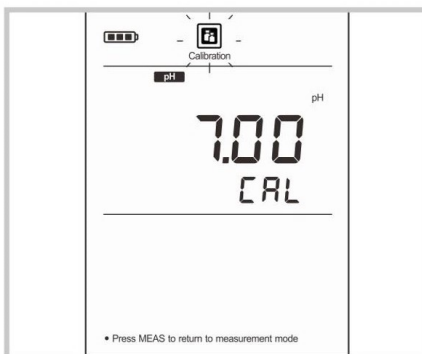


- 1.3 Rinse the pH electrode with distilled water, place the electrode (and temperature probe) into the pH7.00 (or 6.86, or 6.79) buffer solution. The end of the electrode must be completely immersed into the calibration solution. Stir the electrode gently to create a homogeneous solution. Press the **Enter** key, the Calibration icon begins flashing.

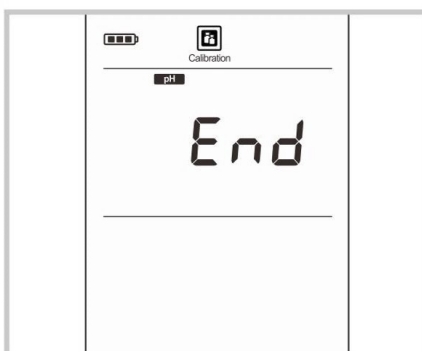


- 1.4 Wait for the reading to stabilize, the meter automatically shows END and returns to the measurement mode. Calibration is completed.


Multi-point calibration

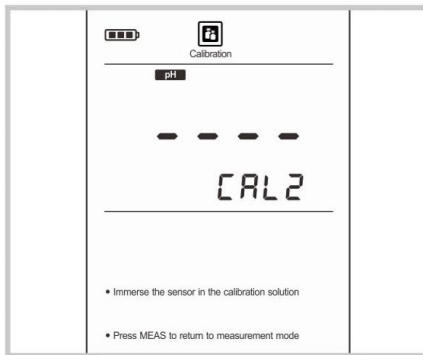

- 2.1 Ensure that you have selected 2 to 5 points calibration in the setup menu.
- 2.2 Repeat the steps 1.2 to 1.3 above. When the first calibration point is completed, the display will show CAL2. The meter prompts you to continue with second point calibration.




- 2.3 Rinse the pH electrode with distilled water, place the electrode (and temperature probe) into the next buffer solution. The meter will automatically recognize the calibration solution (e.g., pH4.01) and begins the calibration, the Calibration icon continuously flashing.




- 2.4 Wait for the reading to stabilize, the display will show CAL3. The meter prompts you to continue with third point calibration.
- 2.5 Repeat the step 2.3 above until the display shows END. The meter automatically returns to the measurement mode. Calibration is completed.


pH calibration with custom buffers

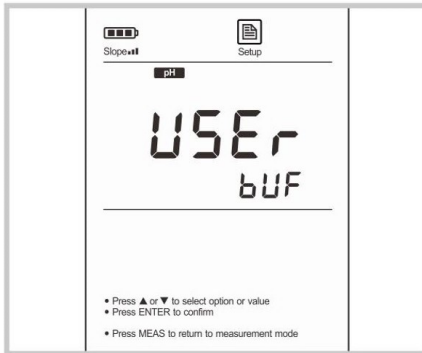


- 3.1 Ensure that you have selected the USER option in the setup menu. The calibration solutions should be at least 1 pH unit apart from each other.
- 3.2 Rinse the pH electrode with distilled water, place the electrode (and temperature probe) into the custom buffer solution. Stir the electrode gently and wait until the measurement is stable.

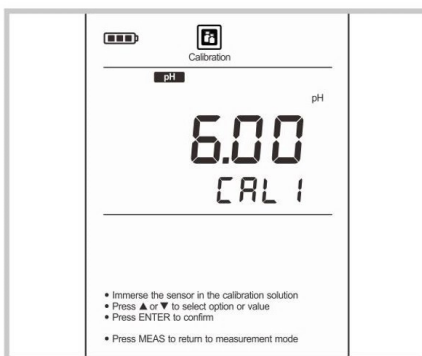

- 3.3 Press the **Cal** key, the meter enters the calibration mode.
- 3.4 If necessary, press the **▲** or **▼** key to set the calibration value, press the **Enter** key to begin the calibration (e.g., 6.00pH).

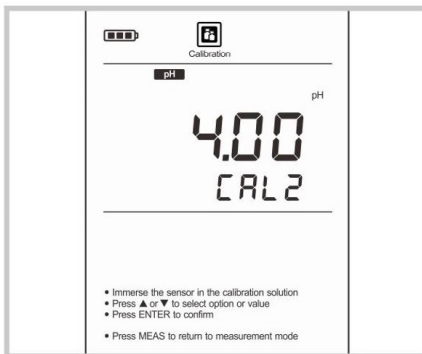

- 3.5 Wait for the reading to stabilize, the display shows CAL2. The meter prompts you to continue with second point calibration.
- 3.6 Rinse the pH electrode with distilled water, place the electrode (and temperature probe) into the next buffer solution and wait until the measurement is stable.
- 3.7 If necessary, press the **▲** or **▼** key to set the calibration value, press the **Enter** key to begin the calibration (e.g., 4.00pH).

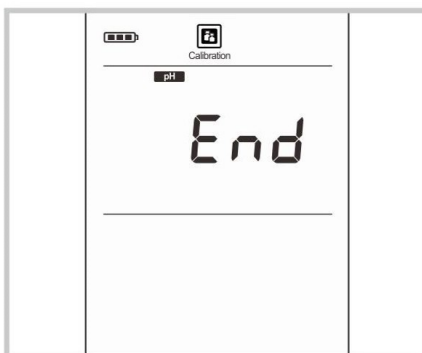


- 3.8 Wait for the reading to stabilize, the meter automatically shows END and returns to the measurement mode. Calibration is completed.




- During the calibration process, if the meter shows **Err**, please check the pH electrode and ensure the pH buffers are fresh and uncontaminated.
- If the electrode slope is not within the normal range (< 70% or >110%), the **Slope■■■** icon will disappear on the display.
- If you want to exit the calibration, press the **Meas** key.


Viewing the pH calibration report

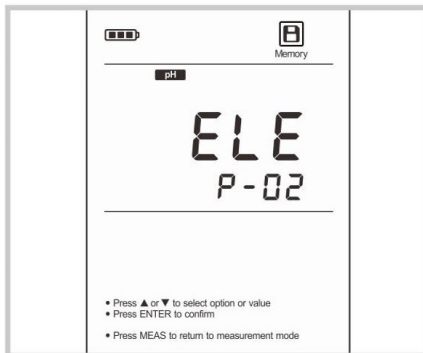


- 4.1 Press the **MR** key in the pH measurement mode, the meter shows LOC/P-01.
- 4.2 Press the **▲** or **▼** key until the meter shows ELE/P-02.

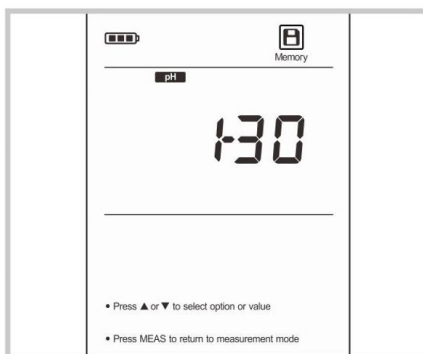

- 4.3 Press the **Enter** key, the meter shows the last calibration date (Format: month-day).



- 4.4 Press the **▼** key, the meter shows the zero-point offset (e.g., 2mV).

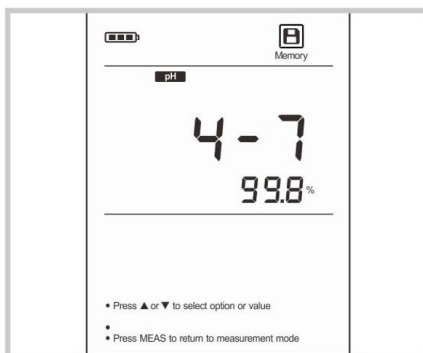


- 4.5 Press the **▼** key, the meter shows the pH buffer group and slope (e.g., pH4~7, slope: 99.8%).
- 4.6 To exit the calibration report, press the **Meas** key.


i If the meter does not calibrated, the display will only show "----".

ORP Calibration


The Bante900P multiparameter water quality meter allows 1 point calibration in the relative mV mode, but calibration is not necessary unless exact readout agreement with a work standard and at a specific ORP value is needed.

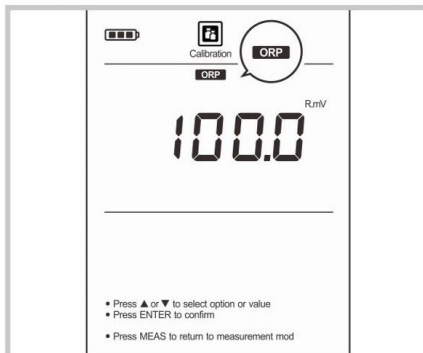

- 1.1 Press the **Mode** key until the meter shows **ORP** icon.
- 1.2 Rinse the ORP electrode with distilled water, place the electrode into the calibration solution. Stir the electrode gently and wait until the measurement is stable.
- 1.3 Press the **Cal** key, the meter enters the calibration mode.




- 1.4 Press the **▲** or **▼** key to set the displayed value (e.g., 105 R.mV).
- 1.5 Press the **Enter** key to confirm, the Calibration icon begins flashing.

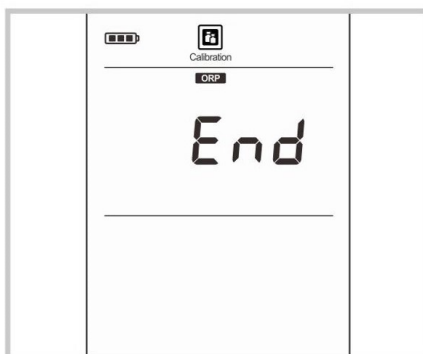


- 1.6 Wait for the reading to stabilize, the meter automatically shows END and returns to the measurement mode. Calibration is completed.


Viewing the ORP calibration report

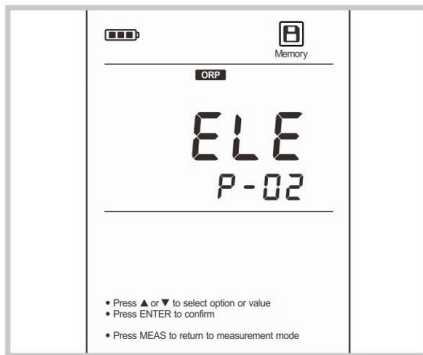

- 2.1 Press the **MR** key in the ORP measurement mode, the display shows LOC/P-01.
- 2.2 Press the ▲ or ▼ key until the display shows ELE/P-02.



- 2.3 Press the **Enter** key, the display shows the last calibration date (Format: month-day).




- 2.4 Press the ▼ key, the display shows the offset potential (e.g., 5mV).
- 2.5 To exit the calibration report, press the **Meas** key.

Ion Concentration Calibration


The Bante900P multiparameter water quality meter is capable of 2 to 5 points ion calibration with standard solutions, available calibration points include the following options.

MEASUREMENT UNITS	CALIBRATION POINTS
ppm	0.001, 0.01, 0.1, 1, 10, 100, 1000, 10000
mg/L	0.001, 0.01, 0.1, 1, 10, 100, 1000, 10000
mol/L	0.001, 0.01, 0.1, 1, 10
mmol/L	0.001, 0.01, 0.1

In order to get accurate measuring results, we recommend that adding the ionic strength adjuster to all standards and samples. A typical addition would be 2ml ISA to 100ml of standards and samples. If the meter does not calibrated or calibration is not successfully, the display will always show 0.000. During the calibration, ensure that the selected calibration points cover the anticipated range of the samples.

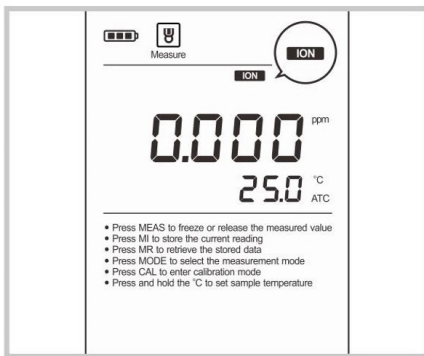


1.1 Press the **Mode** key until the meter shows **ION** icon.

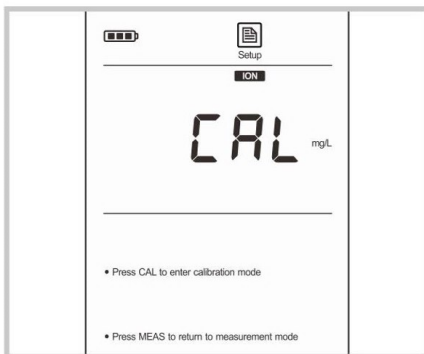


1.2 If necessary, select the concentration unit and ion valence in the setup menu (Refer to page 6 SETUP MENU).

i The meter provides three measurement units, including the ppm, mg/L and mol/L, the factory default is ppm. If the measurement unit has converted, the display will always show "CAL" and wait for calibrating the meter.

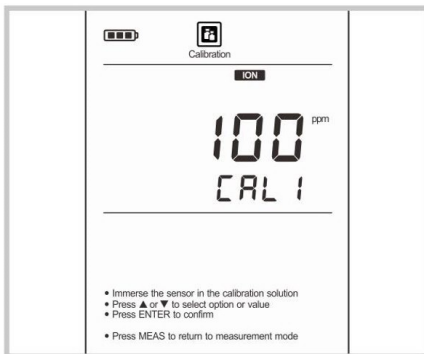


1.3 Press the **Cal** key, the meter enters the calibration mode. The display shows 0.001ppm (or mg/L, mol/L, mmol/L).


1.4 Press the **▲** or **▼** key to select the calibration point (e.g., 100ppm). The meter will automatically perform the calibration from the low to high concentrations.

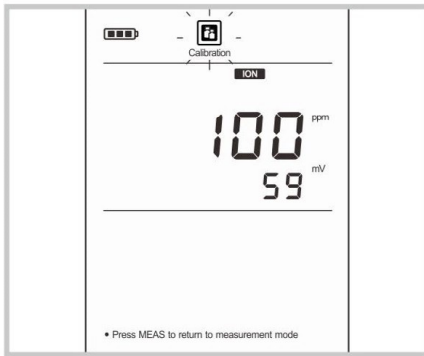


1.5 Rinse the ion selective electrode with distilled water, then rinse with a small amount of standard solution. Place the electrode into corresponding standard solution. Stir the electrode gently to create a homogeneous solution. Press the **Enter** key, the Calibration icon begins flashing.

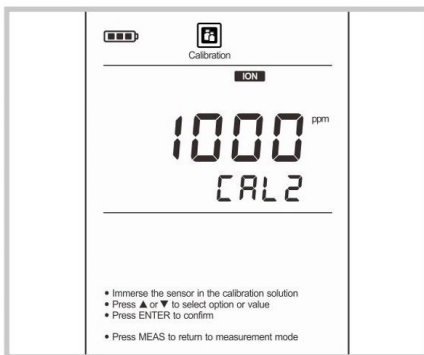

1.6 Wait for the reading to stabilize, the display shows 1000ppm/CAL2. The meter prompts you to continue with second point calibration.

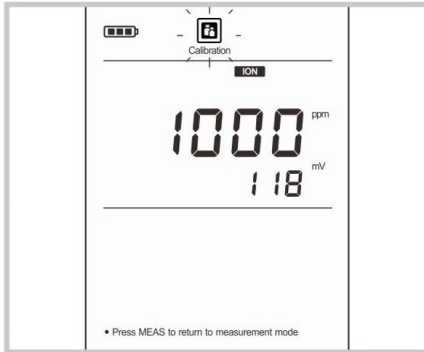

1.7 Rinse the ion selective electrode with distilled water, then rinse with a small amount of standard solution. Place the electrode into the next standard solution. Stir the electrode gently. Press the **Enter** key, the Calibration icon begins flashing.

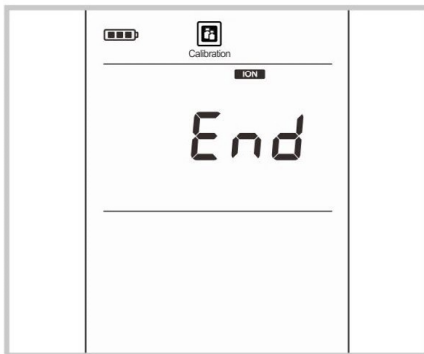


1.8 Wait for the reading to stabilize, the meter automatically show END and return to the measurement mode. Calibration is completed.




- If you have selected the multi-point calibration in the setup menu, the display will show CAL3. The meter prompts you to continue with third point calibration. Repeat the step 1.7 above until the display shows END. The meter will automatically return to the measurement mode.
- If you want to exit the calibration, press the **Meas** key.


Viewing the ion calibration report

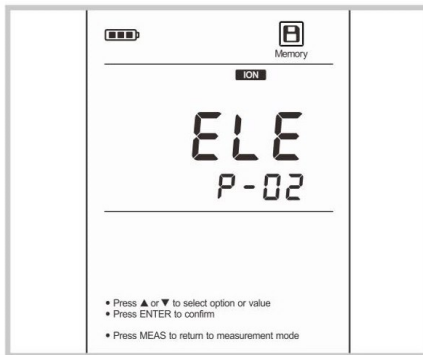


- 2.1 Press the **MR** key in the ion measurement mode, the meter shows LOC/P-01.
- 2.2 Press the **▲** or **▼** key until the meter shows ELE/P-02.



- 2.3 Press the **Enter** key, the meter shows the last calibration date (Format: month-day).



- 2.4 Press the **▼** key, the meter shows the first calibration point and mV value (e.g., 100ppm, 59mV).

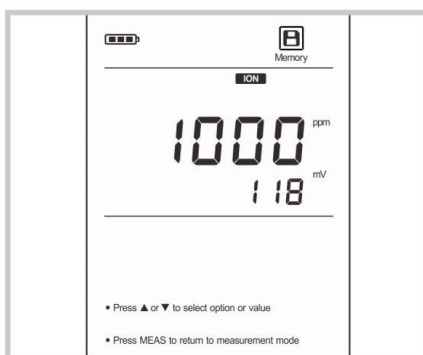

- 2.5 Press the **▼** key, the meter shows the second calibration point and mV value (e.g., 1000ppm, 118mV).
- 2.6 To exit the calibration report, press the **Meas** key.

Selecting the Conductivity Electrode

The Bante900P multiparameter water quality meter is capable of using the 3 types of conductivity electrodes. Prior to the calibration and measurement, you need to select the different sensors as per your sample concentration. The table below shows available electrode and its effective measuring ranges.

CONDUCTIVITY ELECTRODE	MEASURING RANGES	CELL CONSTANT
CON-0.1	0.1~100 μ S/cm	K=0.1
CON-1	10 μ S/cm~10mS/cm	K=1
CON-10	100 μ S/cm~200mS/cm	K=10

Conductivity Calibration - Automatic Calibration


Make sure that you selected the cell constant between 0.1, 1 or 10 in the setup menu. If the current option is "USER", the automatic calibration function will be disabled (Refer to chapter SETUP MENU).

The meter allows 1 to 5 points calibration in the automatic calibration mode. To ensure higher accuracy, we recommend that you perform 3 points calibration or select a standard value close to the sample value you are measuring. The meter will automatically detect these conductivity standard solutions and prompt the user to calibrate the meter. When the calibration is completed, all new calibration values will automatically override existing data.


The following table shows acceptable conductivity range of standard solution for each measuring range.

MEASURING RANGE	CALIBRATION SOLUTION RANGE	DEFAULT
0~20 μ S/cm	7~17 μ S/cm	10 μ S/cm
20~200 μ S/cm	70~170 μ S/cm	84 μ S/cm
200~2000 μ S/cm	700~1700 μ S/cm	1413 μ S/cm
2~20mS/cm	7~17mS/cm	12.88mS/cm
20~200mS/cm	70~170mS/cm	111.8mS/cm


Single point calibration

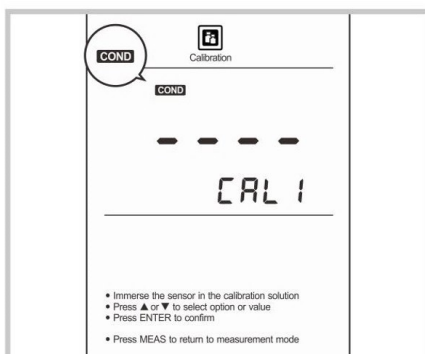


- 1.1 Press the **Mode** key until the meter shows **COND** icon and you have selected 1 point calibration in the setup menu.
- 1.2 Rinse the conductivity electrode with distilled water, then rinse with a small amount of standard solution.
- 1.3 Press the **Cal** key, the display shows "CAL1" and waits for recognizing the standard solution.

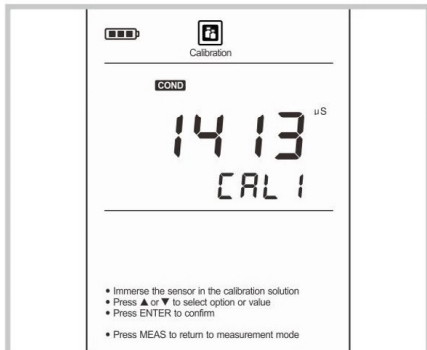

- 1.4 Place the electrode into the conductivity standard solution, the meter automatically shows current calibration standard (e.g., 1413 μ S/cm).
- 1.5 If necessary, press the ▲ or ▼ key to set the calibration value.

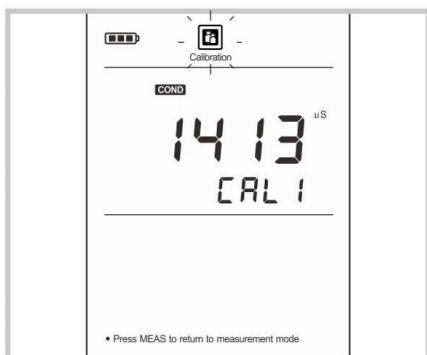

- 1.6 Press the **Enter** key, the Calibration icon begins flashing.

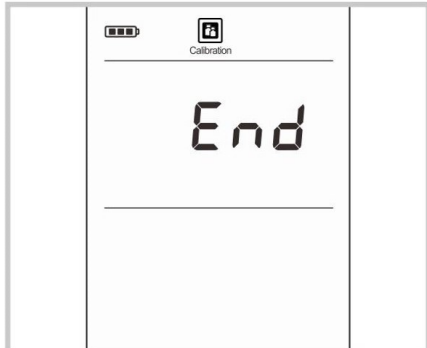

- 1.7 Wait for the reading to stabilize, the display automatically shows END. Single point calibration is completed.


Multi-point calibration

- 2.1 Ensure that you have selected 2 or 5 points calibration in the setup menu.
- 2.2 Repeat steps 1.2 to 1.6 above, when the first calibration point is completed, the display will show "CAL2". The meter prompts you to continue with second point calibration.
- 2.3 Rinse and place the electrode into the standard solution, the display automatically shows current calibration standard (e.g., 12.88mS/cm).
- 2.4 If necessary, press the ▲ or ▼ key to set the calibration value.
- 2.5 Press the **Enter** key, the Calibration icon begins flashing.
- 2.6 Wait for the reading to stabilize, the display will show "CAL3". The meter prompts you to continue with third point calibration.
- 2.7 Repeat the steps 2.3 and 2.5 above until the meter returns to the measurement mode. Calibration is completed.

Conductivity Calibration - Manual Calibration

The Bante900P multiparameter water quality meter provides an easy manual calibration mode. If the conductivity standard solution is not ready, you are able to use this method for calibration.

3.1 Record the cell constant value on the conductivity electrode (e.g., $K=1.01$).

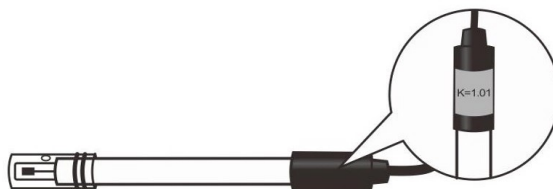


3.2 Press and hold the  key for 3 seconds to enter the setup menu, the display shows "CELL/P-01".

3.3 Press the **Enter** key, the meter enters the setting mode.

3.4 Press the **▲** or **▼** key until the display shows "User/Cell", press the **Enter** key to confirm.


3.5 Press the **▲** or **▼** key to set each digit according to previous record.

3.6 Press the **Enter** key to confirm until the setting values stop flashing. The meter returns to the measurement mode. Calibration is completed.

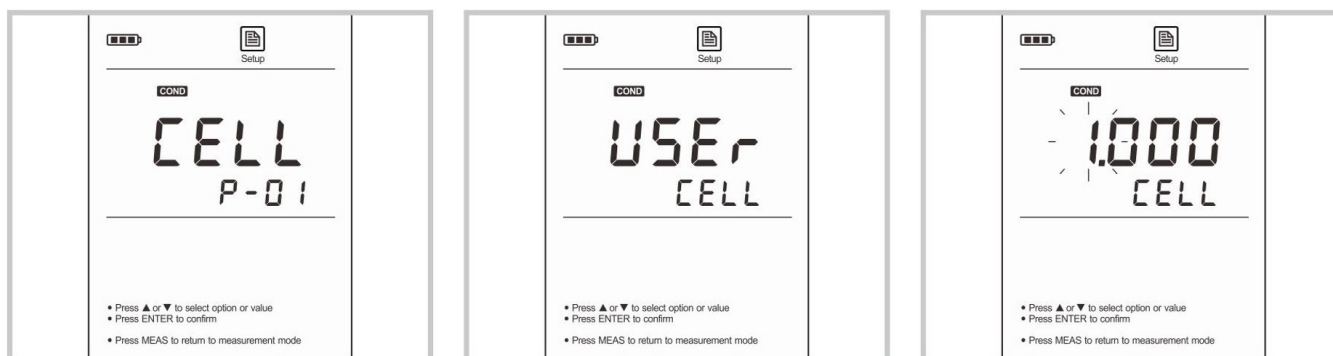


- Performing the conductivity calibration will simultaneously calibrate the corresponding TDS, salinity and resistivity values.
- If you want to exit the calibration, press the **Meas** key.


Viewing the conductivity calibration report

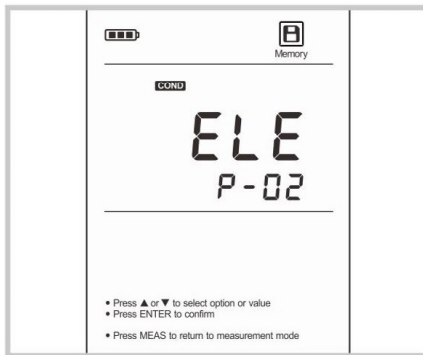

- 4.1 Press the **MR** key in the measurement mode, the display shows LOC/P-01.
- 4.2 Press the **▲** or **▼** key until the display shows ELE/P-02.



- 4.3 Press the **Enter** key, the display shows the last calibration date (Format: month-day).




- 4.4 Press the **▼** key, the display shows the calibration point and calibration factor (e.g., K=0.998).
- 4.5 To exit the calibration report, press the **Meas** key.

DO Calibration in % Saturation Mode

The Bante900P multiparameter water quality meter is able to perform either 1 or 2 points calibration. For single point calibration, we recommend that you perform 100% saturation calibration in the air-saturated water. If the 2 points calibration is selected, the zero oxygen solution needs to be used.


Single point calibration - 100% saturation

- 1.1 Press the **Mode** key until the meter shows **DO** icon and measurement unit "%".
- 1.2 Ensure that you have selected 1 point calibration in the setup menu.
- 1.3 Press the **Cal** key, the meter shows 100.0%/CAL 1.
- 1.4 Hold the dissolved oxygen probe in the air at 100% relative humidity or place the probe into the air-saturated water for 15 minutes. Press the **Enter** key, the meter begins the calibration, the Calibration icon continuously flashing.
- 1.5 Wait for the reading to stabilize, the meter automatically shows END. Calibration is completed.

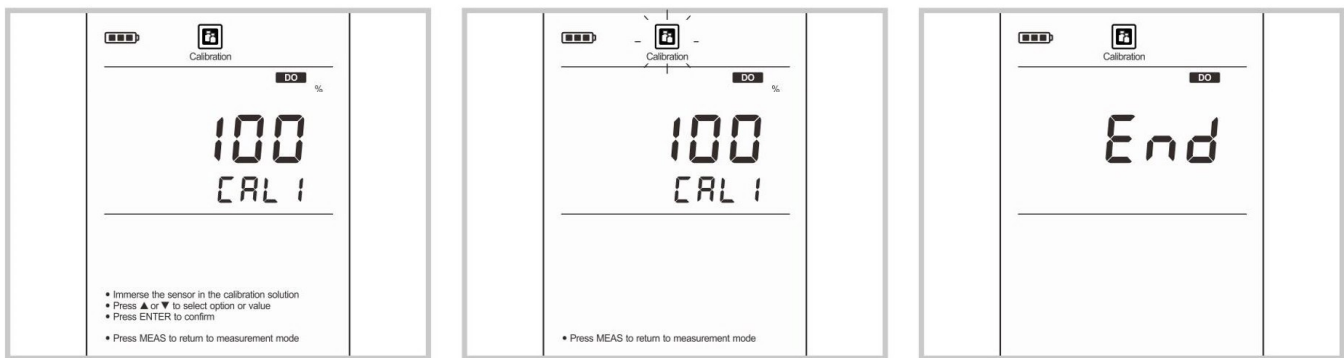

2 points calibration

- 2.1 Ensure that you have selected 2 point calibration in the setup menu.
- 2.2 Press the **Cal** key, the meter shows 100.0%/CAL 1, press the **▲** or **▼** key until the display shows 0/CAL1.
- 2.3 Immerse the dissolved oxygen probe into the zero oxygen solution for at least 10 minutes. Press the **Enter** key, the meter begins the calibration, the Calibration icon continuously flashing.
- 2.4 Wait for the reading to stabilize, the display will show "100%/CAL2", the meter prompts you to continue with second point calibration.
- 2.5 Immerse the dissolved oxygen probe into the air-saturated water for 15 minutes, press the **Enter** key to confirm. Wait for the reading to stabilize, the meter automatically shows END. Calibration is completed.

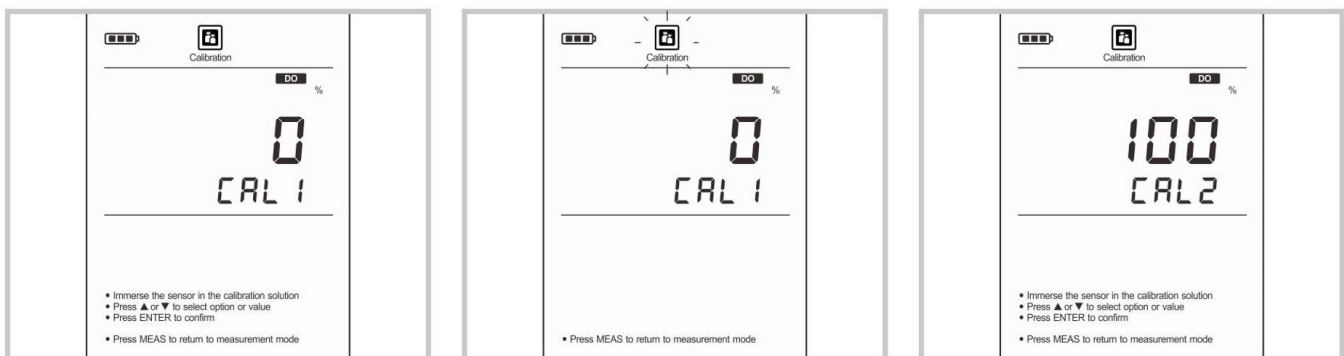


i Performing a percentage saturation calibration will simultaneously calibrate the corresponding mg/L (or ppm) concentration value. Therefore, additional mg/L calibration is not required in most circumstances.

DO Calibration in mg/L or ppm Mode


Single point calibration - air-saturated water

- 1.1 Press the **Mode** key until the meter shows **DO** icon and measurement unit "mg/L or ppm".
- 1.2 Ensure that you have selected 1 point calibration in the setup menu.
- 1.3 Press the **Cal** key, the meter shows 8.25mg/L/CAL 1 (@25°C).
- 1.4 Immerse the dissolved oxygen probe into the air-saturated water for 15 minutes. Press the **Enter** key, the meter begins the calibration, the Calibration icon continuously flashing.
- 1.5 Wait for the reading to stabilize, the meter automatically shows END. Calibration is completed.

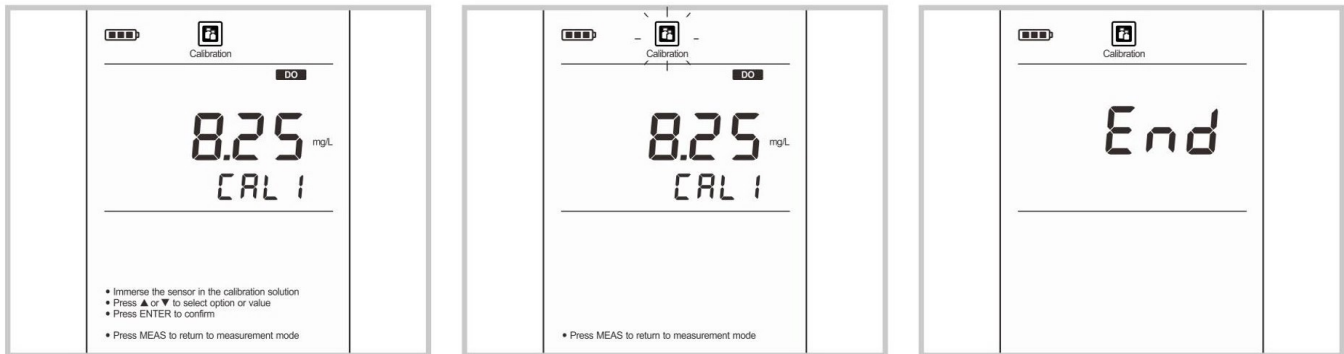

2 points calibration

- 2.1 Ensure that you have selected 2 point calibration in the setup menu.
- 2.2 Press the **Cal** key, the meter shows 8.25mg/L/CAL 1 (@25°C), press the **▲** or **▼** key until the display shows 0.00mg/L/CAL1.
- 2.3 Immerse the dissolved oxygen probe into the zero oxygen solution for at least 10 minutes. Press the **Enter** key, the meter begins the calibration, the Calibration icon continuously flashing.
- 2.4 Wait for the reading to stabilize, the display will show "8.25mg/L/CAL 2", the meter prompts you to continue with second point calibration.
- 2.5 Immerse the dissolved oxygen probe into the air-saturated water for 15 minutes, press the **Enter** key to confirm. Wait for the reading to stabilize, the meter automatically shows END. Calibration is completed.

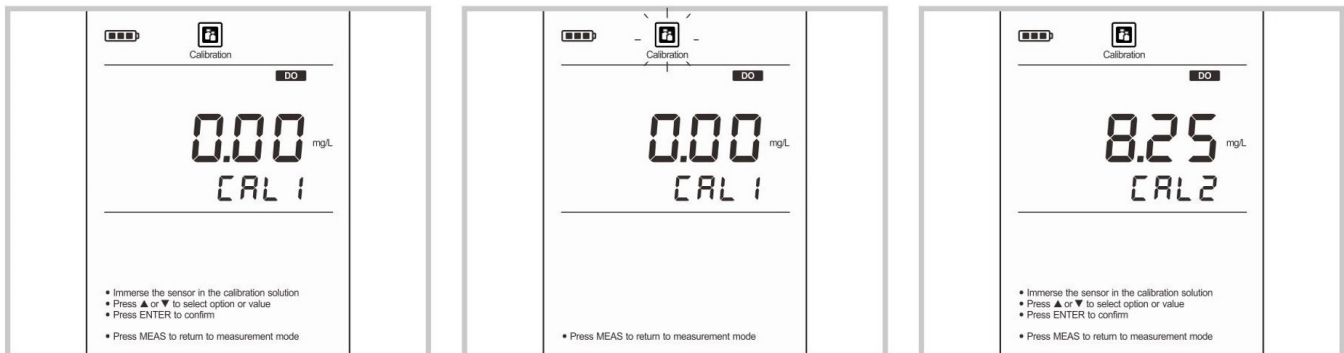


i If you want to exit the calibration, press the **Meas** key.

Temperature Calibration

During the measurement process, if the temperature reading displayed differs from that of an accurate thermometer, the meter needs to be calibrated.

1. Connect the temperature probe to the meter and place into a solution with a known accurate temperature.
2. Press and hold the °C key for 3 seconds to enter the temperature setting mode.
3. Press the ▲ or ▼ key to set the temperature value.
4. Press the **Enter** key to confirm. Calibrating is completed.

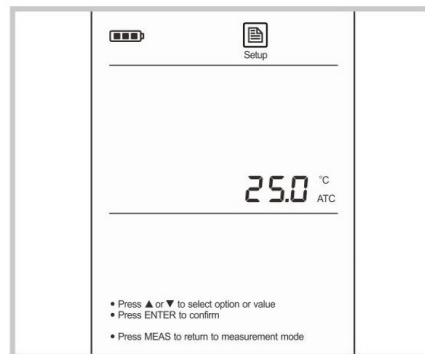

- ① During the setting process, press the ▲ or ▼ key once, the setting value will increase or decrease by 0.1. Press and hold the ▲ or ▼ key, the setting value will increase or decrease by 1.


pH Measurement

1. Press the **Mode** key until the display shows **pH** icon.
2. Rinse the pH electrode with distilled water. Place the electrode (and temperature probe) into the sample solution, stir the electrode gently.
3. Record the measured value when the reading is stable.

ORP Measurement

The Bante900P multiparameter water quality meter provides two millivolt measurement modes.

- Press the **Mode** key until the display shows measurement unit "mV", the meter is now enters the absolute mV measurement mode.
- Press the **Mode** key until the display shows **ORP** icon, the meter is now enters the relative mV measurement mode.

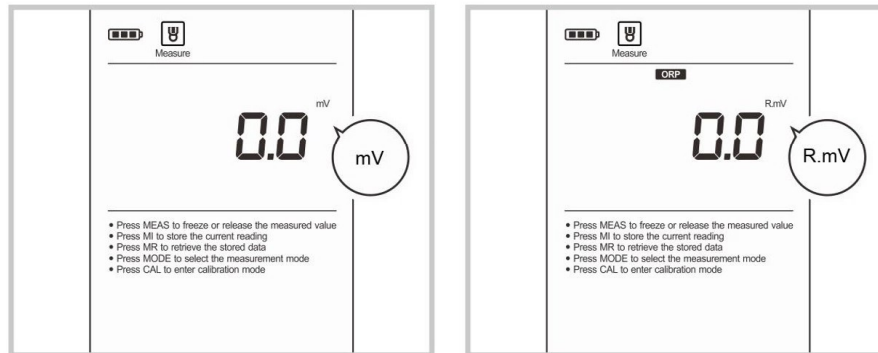

- Select one of the above modes. Place the ORP electrode into the sample. Record the measured value when the reading is stable.

Ion Concentration Measurement

Before measuring, ensure that the temperature of samples are the same as the standard solutions, the maximum error should be controlled within the 1°C. For low level measurements or samples contain the interference ions, adding the ionic strength adjuster to sample and using the plastic beaker are necessary.

1. Press the **Mode** key until the display shows **ION** icon.
2. Rinse the ion selective electrode thoroughly with distilled water. Place the electrode into the sample solution, stir the electrode gently.
3. Record the measured value when the reading is stable.

Conductivity/TDS/Resistivity Measurement

1. Press the **Mode** key until the meter shows **COND** (Conductivity) or **TDS** (TDS) or **RES** (Resistivity) icon.
2. Rinse the conductivity electrode thoroughly with distilled water.
3. Place the electrode into the sample solution, stir the electrode gently.
4. Record the measured value when the reading is stable.

Salinity Measurement

The Bante900P multiparameter water quality meter provides two salinity measurement modes - practical salinity (unit: PSU) and natural seawater (unit: ppt).

1. Press the **Mode** key until the display shows **SAL** icon and measurement unit "PSU", the meter enters the practical salinity measurement mode.
2. If necessary, press the **Mode** key again, the meter shows **SAL** icon and measurement unit "ppt", the meter enters the seawater measurement mode.
3. Select the desired measurement mode. Place the electrode into the sample solution, stir the electrode gently.
4. Record the measured value when the reading is stable.






Dissolved Oxygen Measurement


The meter is suitable for measuring the water, wastewater, brine and other liquids. If the sample is belong to the seawater or other water containing large amounts of salt, please setting the salinity coefficient before measurement. Some gas and steam such as chloride, sulfur dioxide, sulfured hydrogen, ammonium, carbon dioxide and iodine can permeate the membrane via diffusion. So their existence will influence the measurement of dissolved oxygen. If the sample contains the solvent, grease, sulfide and alga, the membrane on the probe will be blocked, damaged or eroded.

Setting the barometric pressure

The following table describes the relationship between altitude and barometric pressure. Prior to the calibration or measurement, you need to set the compatible parameter according to the local altitude.



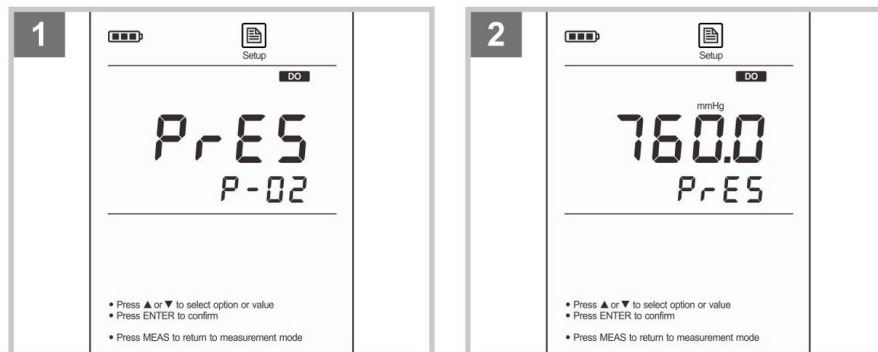


ALTITUDE (m)	kPa	mmHg	ALTITUDE (m)	kPa	mmHg
0	101.3	760	1600	82.9	622
100	100.1	750	1700	81.9	614
200	98.8	741	1800	80.9	607
300	97.6	732	1900	79.9	599
400	96.4	723	2000	78.9	592
500	95.2	714	2100	77.9	584
600	94.0	705	2200	76.9	577
700	92.8	696	2300	76.0	570
800	91.7	688	2400	75.0	563
900	90.5	679	2500	74.1	556
1000	89.4	671	2600	73.2	549
1100	88.3	662	2700	72.3	542
1200	87.2	654	2800	71.4	536
1300	86.1	646	2900	70.5	529
1400	85.0	638	3000	69.6	522
1500	84.0	630	3100	68.7	515


1. Press and hold the  key for 3 seconds to enter the setup menu and the  or  key until the meter shows PRES/P-02.
2. Press the **Enter** key, the meter shows the default barometric pressure.
3. Press the  or  key to set the value, press the **Enter** key to confirm. Setting is completed.



Setting the salinity coefficient

Salt dissolved in water will influence oxygen content of water. If your sample belongs to high concentration liquids, please make sure that you have selected an applicable salinity coefficient before measurement. For the low concentration liquids, please use the default coefficient 0.0 ppt.

1. Press and hold the  key for 3 seconds to enter the setup menu and the  or  key until the meter shows SAL/P-03.
2. Press the **Enter** key, the meter shows the default salinity coefficient (0.0 g/L).
3. Press the  or  key to set the salinity of sample, press the **Enter** key to confirm. Setting is completed.

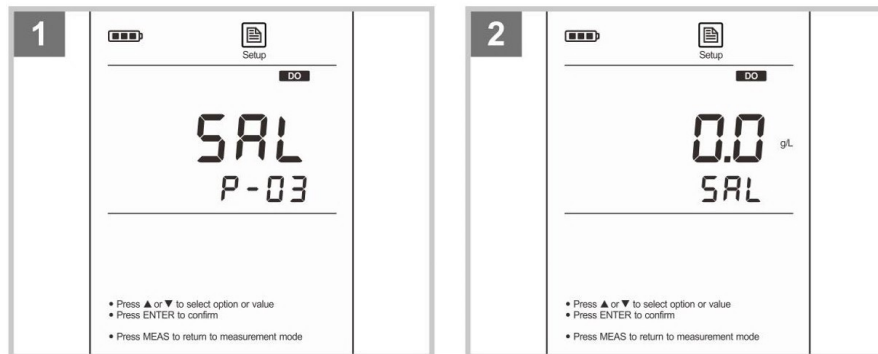


Measurement


1. Connect the dissolved oxygen probe to meter and wait for 15 minutes to polarize the probe.
2. If necessary, to set the barometric pressure and salinity coefficient in the setup menu.
3. Immerse the probe in the sample solution, make sure the temperature sensor on the probe is fully immersed.
4. Stir the probe gently. Record the measured value when the reading is stable.




Temperature sensor

Auto-Hold

The meter contains an Auto-Hold function. If enabled, the meter will automatically sense a stable reading and lock the measurements, the HOLD icon appears on the display. If disabled, press the  key, the meter will immediately lock the displayed value. Press the **Meas** key to resume measuring.

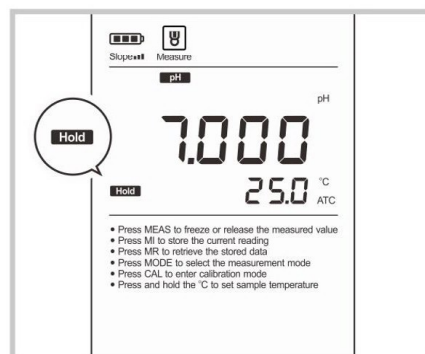


Storing and Recalling Data

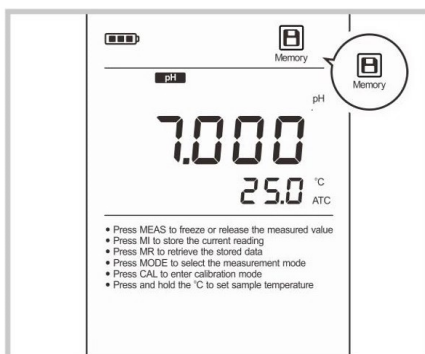

The Bante900P multiparameter water quality meter is capable of storing and recalling up to 500 data sets.


Storing readings into memory

During the measurement process, press the **MI** key to store the reading into the memory, the Memory icon appears on the display.

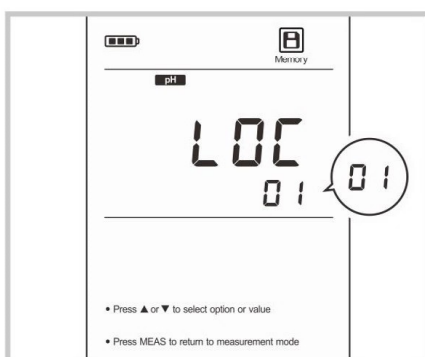


Viewing stored readings

1. Press the **MR** key in the measurement mode, the meter shows LOC/P-01 (Data Log).
2. Press the **Enter** key, the meter shows the serial number of the stored data.

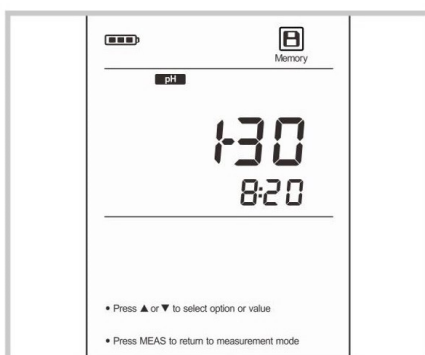

3. Press the ▼ key, the meter shows the date and time of the stored data (Format: month-day, hour-minutes).

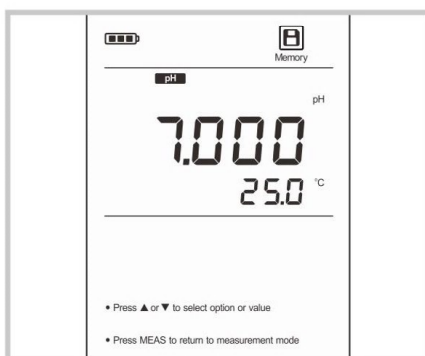

4. Press the ▼ key, the meter shows the stored data.
5. Press the ▼ key again, the meter shows next data set.
6. Press the **Meas** key, the meter returns to the measurement mode.

Clearing the memory


Please refer to page 6 SETUP MENU.

Communication

Bante Instruments provides a Data Acquisition System that can be used to transfer data, receive the measuring values or import the data to Excel. You are able to download this software from our official website at www.banteinstruments.com. Before installation, ensure that Windows 7/8/10 operating system has been installed on your computer.

Receiving data

- Connect the USB cable to meter and computer. Click the DAS icon, the system will automatically scan an available communication port and show the message box "Found a port on your computer".
- Click the **OK** button, the application starts.

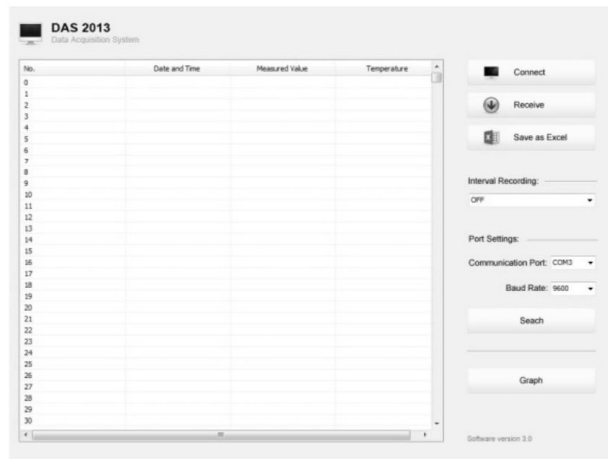

- Click the **Connect** button, the screen shows "Port is connected" indicate that the communication between the meter and the computer has been established.
- Click the **OK** button to confirm.
- Click the **Receive** button, the stored data automatically transfer to computer.

Interval recording

This function is used for recording the measuring value within the specify time period.

- Click the **Interval Recording** button and select a time option.
- Click the **Receive** button, the measured value will automatically send to data sheet.



- The first data need 1 minute to be shown on screen.
- Do not press any key on meter during the Interval Recording mode, it will cause communication interruption.

Graph mode

This function is used for viewing the variations of the measured parameter continuously.

Click the **Graph** button, the screen immediately shows the curve graph. To quit current mode, click the **Back** button.

Create the excel file

When the transfer is completed, click the **Save as Excel** button, the measured values in the data sheet will automatically convert to Excel file.



- Once the software is closed, all received data will be lost and can not be recovered.

Electrode Care and Maintenance

pH electrode

Since pH electrode is susceptible to dirt and contamination, clean as necessary depending on the extent and condition of use.

- After measuring: rinse the electrode in distilled water, store the electrode into the 3M KCL solution.
- Salt deposits: soak the electrode in warm tap water to dissolve deposits, then thoroughly rinse with distilled water.
- Oil or Grease film: wash the glass sensitive membrane of electrode gently in some detergents and water. If necessary, using the alcohol to clean the sensitive membrane, then rinse with distilled water. Place the electrode in the 3M KCL solution for at least 30 minutes.
- Clogged reference junction: heat a diluted KCl solution to 60°C to 80°C. Place the electrode into the heated solution for about 10 minutes. Allow the electrode to cool in some unheated KCl solution.
- Protein deposits: prepare a 1% pepsin solution in 0.1M of HCL. Place the electrode in the solution for 10 minutes. Rinse the electrode with distilled water.

Reactivating the pH Electrode:

If stored and cleaned properly, the electrode should be ready for immediate use. However, a dehydrated sensitive membrane may cause sluggish response. To rehydrate the sensitive membrane, immerse the electrode in a pH4.01 buffer solution for 10 to 30 minutes. If this fails, the electrode requires activation.

1. Soak the electrode in 0.1M HCl for 5 minutes.
2. Remove and rinse with deionized water, then place in 0.1M NaOH for 5 minutes.
3. Remove and rinse again, and soak in 3M KCL solution for at least 30 minutes.

ORP electrode

- Ensure that the ORP electrode is thoroughly washed with distilled water after use.
- In aggressive chemicals, dirty or viscous solutions, and solutions with heavy metals or proteins, take readings quickly and rinse electrode immediately.
- If you do not use the electrode for long periods, store the electrode with 4M KCL solution.

Cleaning the Electrode:

Contamination of the sensing element often results in slow response and inaccurate readings. If necessary, clean the element by one of the following procedures.

Inorganic Deposits:

- 1.1 Soak the ORP electrode in 0.1M HCl for 10 minutes.
- 1.2 Remove and rinse with distilled water, then place in alcohol for 5 minutes.
- 1.3 Remove and rinse again, and soak in pH4.01 buffer solution for 15 minutes.

Oil and Grease Films:


- 2.1 Wash the electrode gently in some detergents and water.
- 2.2 Dip the electrode in the 4M KCL solution for at least 30 minutes.

Ion selective electrode

- Ensure that the electrode is thoroughly washed with distilled water after use.
- DO NOT scratch the sensitive membrane on electrode.
- If you do not use the electrode for long periods, store the electrode in a dry, cool and well-ventilated area.


Conductivity electrode

- DO NOT touch the measurement area of electrode and always make sure that is clean.
- If there is a build-up of solids inside the measurement area, these should be removed very carefully with a cotton bud soaked in solvent, taking care not to touch the metal parts of the inner cell. After the solids are removed, the electrode must be recalibrated.

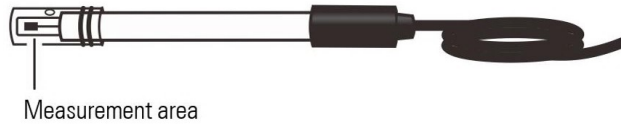

Dissolved oxygen probe

- Always keep the membrane of the dissolved oxygen probe is wet or moist.
- If you do not use the probe for long periods, please screw off membrane cap and rinse the cathode, anode and membrane with deionized water, then soak up residual water on them with filter paper. Install the probe again.

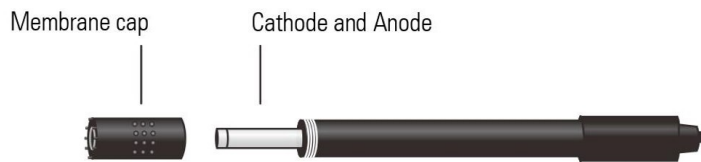

Troubleshooting

LCD DISPLAY	CAUSE	CORRECTIVE ACTION
---	Electrode dried out	Soak the pH electrode in 3M KCL solution at least 30 minutes.
		Soak the ion selective electrode in 100ppm standard solution for 2 hours.
	Measured value is out of range	Soak the conductivity electrode in tap water for a few minutes.
Err	Incorrect calibration solutions	Check the electrode whether clogged, dirty or broken.
	Setting value does not match calibration solution	Using the fresh calibration solutions for calibration.
	DO electrolyte solution is depleted	Reset the calibration value.
	Zero oxygen solution is contaminated	Refilling electrolyte solution.
	pH electrode has expired	Replace the calibration solution.
	Keypad is not working properly	Replace the pH electrode.
		Replace the batteries.

Specifications

pH	Model	Bante900P
	Range	-2.000~20.000pH
	Accuracy	±0.002pH
	Resolution	0.1, 0.01, 0.001pH
	Calibration Points	1 to 5 points
	pH Buffer Options	USA (pH1.68/4.01/7.00/10.01/12.45)
		NIST (pH1.68/4.01/6.86/9.18/12.45)
		DIN (pH1.09/4.65/6.79/9.23/12.75)
Temperature Compensation	0~100°C, 32~212°F, Manual or Automatic	
mV	Range	-1999.9~1999.9mV
	Accuracy	±0.2mV
	Resolution	0.1, 1mV
	Calibration Points	1 point (Only for relative mV mode)
Ion	Range	0.001~19999ppm, mg/L, mol/L (Depending on range of ISE)
	Accuracy	±0.5% F.S (Monovalent), ±1% F.S (Divalent)
	Resolution	0.001, 0.01, 0.1, 1
	Calibration Points	2 to 5 points
	Calibration Solutions	0.001, 0.01, 0.1, 1, 10, 100, 1000, 10000ppm, mol/L, mg/L
	Temperature Compensation	0~100°C, 32~212°F, Manual or Automatic
Conductivity	Range	0.01~20.00, 200.0, 2000µS/cm, 20.00, 200.0mS/cm
	Accuracy	±0.5% F.S
	Calibration Points	1 to 5 points
	Calibration Solutions	10µS/cm, 84µS/cm, 1413µS/cm, 12.88mS/cm, 111.8mS/cm
	Temperature Compensation	0~100°C, 32~212°F, Manual or Automatic
	Temperature Coefficient	0.0~10.0%/°C
	Compensation Modes	Linear or Pure Water
	Cell Constant	K=0.1, 1, 10 or User-defined
	Reference Temperature	20°C or 25°C
TDS	Range	0~10.00, 100.0, 1000ppm, 10.00, 100ppt (Max. 200ppt)
	Accuracy	±1% F.S
	TDS Factor	0.1~1.0 (Default 0.5)

Salinity	Range	0.00~80.00ppt, 0.00~42.00psu
	Accuracy	±1% FS
	Resolution	0.01
	Measurement Modes	Practical Salinity (psu) or Natural Seawater (ppt)
Resistivity	Range	0.00~20.00MΩ
	Accuracy	±1% FS
	Resolution	0.01, 0.1, 1
Dissolved Oxygen	Range	0.00~20.00mg/L
	Accuracy	±0.2mg/L
	Resolution	0.01, 0.1mg/L
	Calibration Points	1 or 2 points
	Temperature Compensation	0~50°C, 32~122°F, Automatic
	Pressure Correction	60.0~112.5kPa, 450~850mmHg
	Salinity Correction	0~50g/L
% Saturation of Oxygen	Range	0.0~200.0%
	Accuracy	±2.0%
	Resolution	0.1, 1%
Temperature	Range	0~105°C, 32~221°F
	Accuracy	±0.5°C
	Resolution	0.1°C
	Calibration Points	1 point
General	Memory	Stores up to 500 data sets
	Output	USB communication interface
	Connector	BNC, 6-pin
	Display	LCD
	Operating Temperature	0~60°C
	Relative Humidity	< 80%
	Power Requirements	3 × 1.5V "AA" batteries
	Dimensions	170 (L) × 85 (W) × 30 (H)mm
	Weight	300g

Addendum 1: pH Electrode Selection Guide

The Bante900P multiparameter water quality meter comes with a general purpose pH electrode that is used to measure the pH of the liquids. If this electrode can not meet your measurement requirements, please refer to the table below to select an applicable probe.

SAMPLE TYPE	P11	P12	P13	P15	P16	P18	P19	P21	E201	E202
Agar										•
Beer	•	•	•					•	•	•
Blood Products	•	•	•					•		•
Bread, Dough						•	•			
Cement	•									
Cosmetics	•	•	•					•	•	•
Dairy Products	•	•	•				•			•
Education	•								•	•
Fats/Cream							•			
Field Use						•			•	•
Fish Products							•			•
Lab Flasks		•								
Low Ionic	•			•				•		
Meat, Cheese							•			•
Micro Samples			•							
Paint		•	•							•
Photographic										
Soil						•	•			
Surface										•
Test Tubes		•			•					
Tris Buffer					•					
Viscose Samples										•

Addendum 2: ORP Electrode Selection Guide


ORDER CODE	APPLICATION
501	Suitable for the sample with strong redox potential, plastic body, temperature range: 0~80°C
502	Suitable for the sample with weak redox potential, plastic body, temperature range: 0~80°C
504	Suitable for the high temperature samples, glass body, temperature range: 0~100°C

Addendum 3: Ion Selective Electrode Selection Guide

ORDER CODE	ION TYPE	RANGE
F-US	Fluoride (F ⁻)	0.02ppm~Saturation
CL-US	Chloride (Cl ⁻)	1.8~35500ppm
Br-US	Bromide (Br ⁻)	0.4~79900ppm
Cn-US	Cyanide (Cn ⁻)	0.2~260ppm
Na-US	Sodium (Na ⁺)	0.1~23000ppm
NO3-US	Nitrate (NO ₃ ⁻)	0.4~62000ppm
Ca-US	Calcium (Ca ²⁺)	0.02~40000ppm
NH4-US	Ammonium (NH ₄ ⁺)	0.1~18000ppm
Cd-US	Cadmium (Cd ²⁺)	0.01~11200ppm
Cu-US	Cupric (Cu ²⁺)	0.006~6400ppm
I-US	Iodide (I ⁻)	0.06~127000ppm
Pb-US	Lead (Pb ²⁺)	0.2~20700ppm
K-US	Potassium (K ⁺)	0.04~39000ppm
Ag-US	Silver (Ag ⁺)	0.01~107900ppm
S-US	Sulphide (S ²⁻)	0.003~32100ppm
NH3-US	Ammonia (NH ₃)	0.02~17000ppm

Addendum 4: Preparation of pH Buffer Solutions

- Open the pH7.00 buffer packet, place the reagent into a 250ml volumetric flask. Pour the distilled water 250ml to scale line, mix the solution until the reagent is completely dissolved.
- Preparation of pH4.01 and 10.01 standard buffer solutions are the same as above. Prepared standard buffer solutions should be stored in hermetically sealed glass containers.

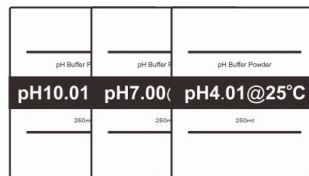

Addendum 5: Preparation of ORP Standard Solutions

- Add 3 grams of quinhydrone to 500ml buffer pH4.01 and stir for 15 minutes. Un-dissolved quinhydrone powder must be present.
Potential @ 25°C =+263mV (±10mV)
- Add 3 grams of quinhydrone to 500ml buffer pH7.00 and stir for 15 minutes. There must be an excess of undissolved quinhydrone powder.
Potential @ 25°C =+87mV (±10mV)

Addendum 6: Preparation of Ion Standard Solutions (1000ppm)

To prepare these solutions, half fill a 1 liter volumetric flask with distilled water and add the analytical grade reagent below.

ION TYPE	REAGENT	WEIGHT
Fluoride (F ⁻)	Sodium Fluoride	2.21g
Chloride (Cl ⁻)	Sodium Chloride	1.65g
Bromide (Br ⁻)	Sodium Bromide	1.29g
Cyanide (Cn ⁻)	Sodium Cyanide	1.88g
Sodium (Na ⁺)	Sodium Chloride	2.542g
Nitrate (NO ₃ ⁻)	Sodium Nitrate	1.37g
Calcium (Ca ²⁺)	Calcium Chloride	3.67g
Ammonium (NH ₄ ⁺)	Ammonium Chloride	2.97g
Cadmium (Cd ²⁺)	Cadmium Nitrate	2.74g
Cupric (Cu ²⁺)	Copper Nitrate	3.80g
Iodide (I ⁻)	Sodium Iodide	1.18g
Lead (Pb ²⁺)	Lead Perchlorate	2.22g
Potassium (K ⁺)	Potassium Chloride	1.91g
Silver (Ag ⁺)	Silver Nitrate	1.57g
Sulphide (S ²⁻)	Sodium Sulfide	7.49g
Ammonia (NH ₃)	Ammonium Chloride	3.82g

Swirl the flask gently to dissolve the reagent and fill to the mark with distilled water. Cap the flask and upend several times to mix the solution.

Addendum 7: Preparation of Conductivity Standard Solutions

Place AR potassium chloride reagent in a 50ml beaker and dry in an oven for 3 to 5 hours at 105°C, then cool to room temperature in desiccator.

CALIBRATION SOLUTIONS	REAGENT
84µS/cm	Accurately weigh out 42.35mg of KCL and dissolve in 1 litre deionised water.
1413µS/cm	Accurately weigh out 745.9mg of KCL and dissolve in 1 litre deionised water.
12.88mS/cm	Accurately weigh out 7.45g of KCL and dissolve in 1 litre deionised water.
111.8mS/cm	Accurately weigh out 74.5g of KCL and dissolve in 1 litre deionised water.

Stir the solution until the reagent has thoroughly mixed. Preparation is completed.

Addendum 8: How to calculate the temperature coefficient

To determine the temperature coefficient of sample solution use the formula below:

$$T_c = \frac{C_{TB} - C_{TA}}{C_{TA}(T_B - 25) - C_{TB}(T_A - 25)} \times 100\%$$

Where:

T_c = Temperature coefficient

C_{TA} = Conductivity at Temperature A

C_{TB} = Conductivity at Temperature B

T_A = Temperature A

T_B = Temperature B

1. Press and hold the °C key for 3 seconds to enter the temperature setting.
2. Press the ▲ or ▼ key to set the temperature to 25°C.
3. Place the electrode into the sample solution A and record the temperature value T_A and conductivity value C_{TA} .
4. Condition the sample solution and electrode to a temperature that is about 5°C to 10°C different from T_A . Record the temperature value T_B and conductivity value C_{TB} .
5. Calculate the temperature coefficient according to the formula above.

Addendum 9: How to calculate the TDS conversion factor

To determine the TDS conversion factor use the formula below:

$$\text{Factor} = \frac{\text{Actual TDS}}{\text{Actual Conductivity @ 25°C}}$$

Where:

Actual TDS: value from the high purity water and precisely weighed NaCl or KCL reagent.

Actual Conductivity: the meter measured conductivity value.

For example: dissolve 64g of potassium chloride reagent in 1 litre distilled water. If its conductivity value is 100mS/cm, then TDS conversion factor is 0.64.

Addendum 10: Preparation of the Zero Oxygen Solution

Dissolve 500mg of sodium sulfate (Na_2SO_3) reagent and a small amount of cobalt(II) chloride hexahydrate ($\text{CoCl}_2 \cdot 6\text{H}_2\text{O}$) in the 250mL distilled water, mix the solution until the reagent is completely dissolved.

Hazardous Substance Statement

Instruments is committed to the reduction and eventual elimination of all hazardous substances in both the manufacturing process and finished products we supply. We have an active manufacturing and procurement program to minimize and eliminate the use of harmful heavy metals such as cadmium, lead, mercury and the like. New technologies and design parameters are also promoting these efforts and we expect to have little or no such materials in our product in the coming years. We welcome our customer suggestions on how to speed up these efforts.



Warranty

The warranty period for meter is one year from the date of shipment. Above warranty does not cover the sensor and calibration solutions. Out of warranty products will be repaired on a charged basis. The warranty on your meter shall not apply to defects resulting from:

- Improper or inadequate maintenance by customer.
- Unauthorized modification or misuse.
- Operation outside of the environment specifications of the products.

For more information, please contact the nearest authorized distributor.